Aesculap Endoscopic Technology





DISASSEMBLY




Deactivate ratchet on ratchet handle

Flip down red toggle switch. N.B.: for PO959R only



Remove shaft from handle

Remove the shaft by pulling the instrument shaft out of the handle.



Disassemble shaft II


Hold the jaw insert at the tip and remove the inner metal tube.



Disconnect shaft and handle

Pull rotation knob back until it locks in place. A red ring becomes visible.

Important: Do not hold on to the movable handle component.



Disassemble shaft I

Hold the jaw insert at the tip and remove the outer insulation tube.



Assemble shaft I


Slide the metal inner tube onto the jaw insert with its four spring tongues towards the working end until the tongues snap in place.



Prepare handle

If the red ring is not visible, pull the rotation knob back. Deactivate the ratchet by flipping down the red toggle switch.

N.B.: for PO959R only



Assemble shaft II

Slide the outer insulation tube as far as it will go over the inner metal tube.



Connect shaft and handle

Hold the shaft firmly by its tip and the handle behind the rotation knob. Push the shaft into the handle until it locks in place and the red ring disappears. Important: Do not hold on to the movable handle component.



inner metal tube

outer insulation tube

- 1 toggle switch
- 2 rotation knob
- 3 movable handle component



Test the assembly of the instrument by opening and closing the handle to ensure the jaw is opening and

Lubricate the defined places on the instruments (instruments jaw and red toggle switch) with Aesculap Sterilit Oil after each cleaning cycle



- Reprocess the product immediately after use
- I The product can be sterilized either in disassembled or in assembled condition
- For advice on cleaning, disinfection and sterilization, please follow the instructions for use
- For the latest information on reprocessing, please also refer to the Aesculap Extranet via www.aesculap-extra.net
- For accessories and spare parts, please refer to Brochure C766 or visit www.endoscopy-catalog.com

In order to ensure the preservation of full guarantee and warranty rights, only persons authorized by Aesculap may carry out repairs.

Please send products for repair to: Aesculap Technical Service, Am Aesculap-Platz, 78532 Tuttlingen, Germany.


Additional service addresses may be obtained from the same address or via ats@aesculap.de

Aesculap Endoscopic Technology

AdTec® monopolar



AESCULAP®

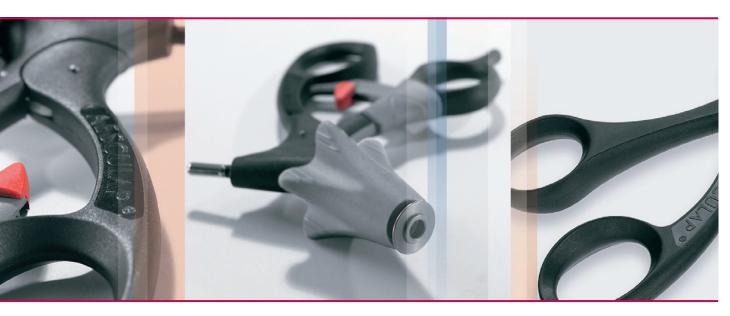

Disassembly and assembly instructions



Aesculap AG & Co. KG

Am Aesculap-Platz 78532 Tuttlingen Germany

Phone +49 7461 95-0 Fax +49 7461 95-2600

www.aesculap.de



All rights reserved. Technical alterations are possible. This leaflet may be used for no other purposes than offering, buying and selling of our products. No part may be copied or reproduced in any form. In the case of misuse we retain the rights to recall our catalogues and pricelists and to take legal actions.

Brochure No. C 222 02 0906/1.0/1